

Human IL-4 ELISA Kit

For the quantitative determination of human interleukin 4 (IL-4) concentrations in serum, plasma, cell culture supernatant, and other biological fluids.

Catalogue Number: EL10026

96 tests

FOR LABORATORY RESEARCH USE ONLY
NOT FOR USE IN DIAGNOSTIC PROCEDURES



ANOGEN

2355 Derry Road East, Unit 23
Mississauga, Ontario
CANADA L5S 1V6
Tel: (905) 677-9221 or (877) 755-8324
Fax: (905) 677-0023

Email: info@anogen.ca ♦ Web Site: www.anogen.ca

S7.5 (04) IL-4

TABLE OF CONTENTS

	Page
INTENDED USE	2
INTRODUCTION	2
PRINCIPLE OF THE ASSAY	3
LIMITATION OF THE PROCEDURE	3
REAGENTS PROVIDED	4
MATERIALS REQUIRED BUT NOT SUPPLIED	5
PRECAUTIONS	5
SAMPLE PREPARATION	6
.....Collection, Handling and Storage	6
PREPARATION OF REAGENTS	6
ASSAY PROCEDURE	8
CALCULATION OF RESULTS	9
TYPICAL DATA	9
.....Example one (Calibrator Diluent I)	10
.....Example two (Calibrator Diluent II)	10
PERFORMANCE CHARACTERISTICS	11
.....Intra-assay precision	11
.....Inter-assay precision	11
.....Recovery	12
.....Sensitivity	12
.....Specificity	12
.....Calibration	12
REFERENCES & CITATIONS	13

INTENDED USE

This Human Interleukin 4 ELISA Kit is to be used for the *in vitro* quantitative determination of human interleukin 4 (IL-4) concentrations in serum, plasma, cell culture supernatant, and other biological fluids. This kit is intended for LABORATORY RESEARCH USE ONLY and is not for use in diagnostic or therapeutic procedures.

INTRODUCTION

Interleukin 4 (IL-4) was initially characterized as a B cell stimulatory factor (BSF-1) (1) and B-cell differentiation factor (BCDF γ) (2). It was subsequently revealed that IL-4 is a pleiotropic cytokine with multiple immune response modulating functions on diverse cell types including T cells, monocytes, macrophages, mast cells, fibroblasts, endothelial cells, osteoblasts, keratinocytes, hepatocytes and astrocytes (3-8). IL-4 is produced by CD4⁺ TH0 and TH2 cells (9,10), fetal thymocytes (11), CD8⁺ T cells (12), mast cells (13) and basophils (14).

Human and mouse cDNAs for IL-4 encode precursor proteins containing 153 and 140 amino acid residues, respectively. The signal peptides from the precursors are cleaved to yield mature proteins of 129 amino acid residues (human) and 120 amino acid residues (mouse) (17, 18). Both human and mouse proteins have multiple potential glycosylation sites and six cysteines that are all involved in intra-molecular disulfide bridges.

IL-4 exhibits approximately 25% amino acid sequence homology to IL-13 that shares a number of biological functions with IL-4 (19). The human and mouse IL-4 gene, each composed of four exons and three introns, have been localized to human chromosome 5q23-31 and mouse chromosome 11 in tandem with genes for IL-3, IL-5, IL-9, IL-13 and GM-CSF (20, 21).

IL-4 is an anti-inflammatory cytokine that exhibits multiple immuno-modulation functions on a variety of cell types, including T cells, B cells, monocytes, neutrophils, hematopoietic progenitors, fibroblasts, endothelial cells, and epithelial cells (15, 16).

The diverse effects exhibited by IL-4 *in vitro* suggest that it may play a central role in the modulation of immune and inflammatory responses *in vivo*. It was reported that introduction of malignant tumor cells transfected with the gene for IL-4 and producing IL-4 in athymic mice can block tumor formation by other transplantable tumor lines *in vivo*. Since the anti-tumor activity of IL-4 is evident in these athymic mice, IL-4-mediated host-defense responses other than T cell immunity must be involved (22). It was reported that IL-4 is important for protective immunity in parasitic nematode-infected mice, since IL-4 or IL-4R antibodies can block the polyclonal IgE response and abrogate protective immunity to the infection (23). In contrast to results obtained with the nematode-infected mice, endogenous IL-4 was reported to inhibit protective immunity in mice infected with the protozoan *Leishmania major* (24, 25). Clearly, much more work is required to unravel

the complex network of IL-4-dependent processes in order to utilize IL-4 successfully in immunotherapy (16).

This IL-4 ELISA is a 4.5 hour solid phase immunoassay readily applicable to measure IL-4 levels in serum, plasma, cell culture supernatant, and other biological fluids in the range of 0 to 1000 pg/mL. It showed no cross reactivity with other cytokines tested. This IL-4 ELISA is expected to be effectively used for further investigations into the relationship between IL-4 and the various conditions mentioned.

PRINCIPLE OF THE ASSAY

This IL-4 enzyme linked immunosorbent assay (ELISA) applies a technique called a quantitative sandwich immunoassay. The microtiter plate provided in this kit has been pre-coated with a polyclonal antibody specific to IL-4. Standards or samples are then added to the appropriate microtiter plate wells with a biotin-conjugated monoclonal antibody preparation specific for IL-4 and incubated. IL-4 if present, will bind and become immobilized by the antibody pre-coated on the wells and then be “sandwiched” by biotin conjugate. The microtiter plate wells are thoroughly washed to remove unbound IL-4 and other components of the sample. In order to quantitatively determine the amount of IL-4 present in the sample, Avidin conjugated to Horseradish Peroxidase (HRP) is added to each microplate well and incubated. Avidin is a tetramer containing four identical subunits that each have a high affinity-binding site for biotin. The wells are thoroughly washed to remove all unbound HRP-conjugated Avidin and a TMB (3,3',5,5' tetramethyl-benzidine) substrate solution is added to each well. The enzyme (HRP) and substrate are allowed to react over a short incubation period. Only those wells that contain IL-4, biotin-conjugated antibody, and enzyme-conjugated Avidin will exhibit a change in colour. The enzyme-substrate reaction is terminated by the addition of a sulphuric acid solution and the colour change is measured spectrophotometrically at a wavelength of 450 nm \pm 2 nm.

LIMITATIONS OF THE PROCEDURE

- FOR LABORATORY RESEARCH USE ONLY, NOT FOR USE IN DIAGNOSTIC PROCEDURES.
- As manufacturers we take great care to ensure that our products are suitable for use with all validated sample types, as designated in the product insert. However, it is possible that in some cases, high levels of interfering factors may cause unusual results.
- The kit should not be used beyond the expiration date on the kit label.
- It is important that the Calibrator Diluent selected for the standard curve be consistent with the samples being assayed.
- If samples generate values higher than the highest standard, dilute the samples with the appropriate Calibrator Diluent and repeat the assay.
- Any variation in standard diluent, operator, pipetting technique, washing technique, incubation time or temperature, and kit age can cause variation in binding.

- Soluble receptors or other binding proteins present in biological samples do not necessarily interfere with the measurement of ligands in samples. However, until the factors have been tested, the possibility of interference cannot be excluded.

REAGENTS PROVIDED

All reagents provided are stored at 2-8°C. Refer to the expiration date on the label.

		96 tests
1.	IL-4 MICROTITER PLATE (Part EL26-1) _____ Pre-coated with anti-human IL-4 polyclonal antibody.	96 wells
2.	BIOTIN CONJUGATE (Part EL26-2) _____ Anti-human IL-4 monoclonal antibody conjugated to Biotin.	6 mL
3.	AVIDIN CONJUGATE (Part EL26-3) _____ Avidin conjugated to horseradish peroxidase.	12 mL
4.	IL-4 STANDARD (Part EL26-4) _____ WHO reference Code8/656 (2ng/vial)	2 vials
5.	CALIBRATOR DILUENT I (Part EL26-5) _____ Animal serum with buffer and preservative. <i>for serum/plasma testing.</i>	25 mL
6.	CALIBRATOR DILUENT II (Part EL26-6) _____ Cell culture medium with calf serum and preservative. <i>For cell culture supernatant testing.</i>	25 mL
7.	WASH BUFFER (20X) (Part 30005) _____ 20-fold concentrated solution of buffered surfactant.	60 mL
8.	SUBSTRATE A (Part EL26-7) _____ Buffered solution with H ₂ O ₂	10 mL
9.	SUBSTRATE B (Part 30007) _____ Buffered solution with TMB.	10 mL
10.	STOP SOLUTION (Part 30008) _____ 2N Sulphuric Acid (H ₂ SO ₄). Caution: Caustic Material!	14 mL

MATERIALS REQUIRED BUT NOT SUPPLIED

1. Single or multi-channel precision pipettes with disposable tips: 10-100 μ L and 50-200 μ L for running the assay.
2. Pipettes: 1 mL, 5 mL 10 mL, and 25 mL for reagent preparation.
3. Multi-channel pipette reservoir or equivalent reagent container.
4. Test tubes and racks.
5. Polypropylene tubes or containers (25 mL).
6. Erlenmeyer flasks: 100 mL, 400 mL, 1 L and 2 L.
7. Microtiter plate reader (450 nm \pm 2nm)
8. Automatic microtiter plate washer or squirt bottle.
9. Sodium hypochlorite solution, 5.25% (household liquid bleach).
10. Deionized or distilled water.
11. Plastic plate cover.
12. Disposable gloves.
13. Absorbent paper.

PRECAUTIONS

1. Do not substitute reagents from one kit lot to another. Standard, conjugate and microtiter plates are matched for optimal performance. Use only the reagents supplied by manufacturer.
2. Allow kit reagents and materials to reach room temperature (20-25°C) before use. Do not use water baths to thaw samples or reagents.
3. Do not use kit components beyond their expiration date.
4. Use only deionized or distilled water to dilute reagents.
5. Do not remove microtiter plate from the storage bag until needed. Unused strips should be stored at 2-8°C in their pouch with the desiccant provided.
6. Use fresh disposable pipette tips for each transfer to avoid contamination.
7. Do not mix acid and sodium hypochlorite solutions.
8. Human serum and plasma should be handled as potentially hazardous and capable of transmitting disease. Disposable gloves must be worn during the assay procedure, since no known test method can offer complete assurance that products derived from human blood will not transmit infectious agents. Therefore, all blood derivatives should be considered potentially infectious and good laboratory practices should be followed.
9. All samples should be disposed of in a manner that will inactivate human viruses.
Solid Wastes: Autoclave 60 min. at 121°C.
Liquid Wastes: Add sodium hypochlorite to a final concentration of 1.0%. The waste should be allowed to stand for a minimum of 30 minutes to inactivate the virus before disposal.
10. Substrate Solution is easily contaminated. If bluish prior to use, *do not use*.
11. Substrate B contains 20% acetone, keep this reagent away from sources of heat or flame.
12. If Wash Buffer (20X) is stored at a lower temperature (2-5°C), crystals may form which must be dissolved by warming to 37°C prior to use.

SAMPLE PREPARATION

COLLECTION, HANDLING, AND STORAGE

- a) **Cell Culture Supernatant:** Centrifuge to remove any visible particulate material.
- b) **Serum:** Blood should be drawn using standard venipuncture techniques and serum separated from the blood cells as soon as possible. Samples should be allowed to clot for one hour at room temperature, centrifuged for 10 minutes (4°C), and serum extracted.
- c) **Plasma:** Blood should be drawn using standard venipuncture techniques and plasma collected using sodium citrate, EDTA, or heparin as an anticoagulant. To ensure optimal recovery and minimal platelet contamination, after collection there must be quick separation of plasma with less than 30 minutes on ice. Centrifuge for 10 minutes (4°C) to remove any particulates.
 - Avoid grossly hemolytic, lipidic or turbid samples.
 - Serum, plasma, and cell culture supernatant samples to be used within 24-48 hours may be stored at 2-8°C, otherwise samples must stored at -20°C to avoid loss of bioactivity and contamination. Avoid freeze-thaw cycles.
 - When performing the assay slowly bring samples to room temperature.
 - It is recommended that all samples be assayed in duplicate.
 - DO NOT USE HEAT-TREATED SPECIMENS.

PREPARATION OF REAGENTS


Remove all kit reagents from refrigerator and allow them to reach room temperature (20-25°C). Prepare the following reagents as indicated below. Mix thoroughly by gently swirling before pipetting. Avoid foaming.

1. **Wash Buffer (1X):** Add 60 mL of Wash Buffer (20X) and dilute to a final volume of 1200 mL with distilled or deionized water. Mix thoroughly. If a smaller volume of Wash Buffer (1X) is desired, add 1 volume of Wash Buffer (20X) to 19 volumes of distilled or deionized water. Wash Buffer (1X) is stable for 1 month at 2-8°C. Mix well before use.
2. **Substrate Solution:** Substrate A and Substrate B should be mixed together in equal volumes up to 15 minutes before use. Refer to the table below for correct amounts of Substrate Solution to prepare.

Strips Used	Substrate A (mL)	Substrate B (mL)	Substrate Solution (mL)
2 strips (16 wells)	1.5	1.5	3.0
4 strips (32 wells)	3.0	3.0	6.0
6 strips (48 wells)	4.0	4.0	8.0
8 strips (64 wells)	5.0	5.0	10.0
10 strips (80 wells)	6.0	6.0	12.0
12 strips (96 wells)	7.0	7.0	14.0

3. **IL-4 Standard:**

- a) Two vials of Standards are provided in this kit to allow both serum/plasma and cell culture supernatant testing. Reconstitute the IL-4 Standard with either 2.0 mL of Calibrator Diluent I (for serum/plasma testing) or Calibrator Diluent II (for cell culture supernatant testing). This reconstitution produces a stock solution of 1000 pg/mL. Allow solution to sit for at least 15 minutes with gentle agitation prior to making dilutions. Use within one hour of reconstituting. The IL-4 standard stock solution can be stored frozen (-20°C) for up to 30 days. Avoid freeze-thaw cycles; aliquot if repeated use is expected.
- b) Use the above stock solution to produce a serial 2-fold dilution series within the range of this assay (31.25 pg/mL to 1000 pg/mL) as illustrated. Add 0.5 mL of the appropriate Calibrator Diluent to each test tube. Between each test tube transfer be sure to mix contents thoroughly. The undiluted IL-4 Standard will serve as the **high standard (1000 pg/mL)** and the Calibrator Diluent will serve as the **zero standard (0 pg/mL)**.

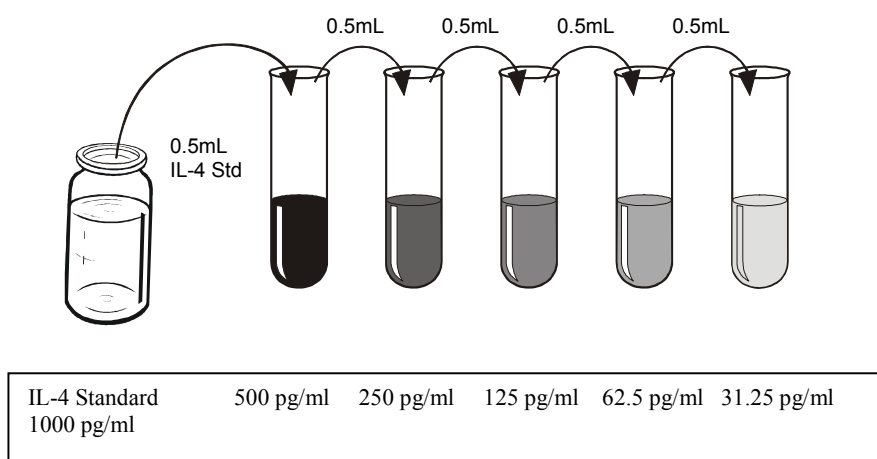

ASSAY PROCEDURE

1. Prepare Wash Buffer (1X) and IL-4 Standards before starting assay procedure (see Preparation of Reagents). *It is recommended that the table and diagram provided be used as a reference for adding Standards or Samples to the Microtiter Plate*

Wells	Contents	Wells	Contents
1A, 1B	Standard 1 0 pg/mL (S1)	2C, 2D	Standard 1 500 pg/mL (S6)
1C, 1D	Standard 2 31.25 pg/ml (S2)	2E, 2F	Standard 1 1000 pg/mL (S7)
1E, 1F	Standard 3 62.50 pg/ml (S3)	2G-12H	IL-4 samples
1G, 1H	Standard 4 125 pg/mL (S4)		
2A, 2B	Standard 5 250 pg/mL (S5)		

	1	2	3	4	5	6	7	8	9	10	11	12
A	S1	S5	2	6	10	14	18	22	26	30	34	38
B	S1	S5	2	6	10	14	18	22	26	30	34	38
C	S2	S6	3	7	11	15	19	23	27	31	35	39
D	S2	S6	3	7	11	15	19	23	27	31	35	39
E	S3	S7	4	8	12	16	20	24	28	32	36	40
F	S3	S7	4	8	12	16	20	24	28	32	36	40
G	S4	1	5	9	13	17	21	25	29	33	37	41
H	S4	1	5	9	13	17	21	25	29	33	37	41

2. Add 100 μ L of Standard or Sample to the appropriate well of the antibody pre-coated Microtiter Plate. Cover and incubate for 1 hour at room temperature.
3. Without discarding the standard and standards, add 50 μ L Anti-IL4 Biotin Conjugate to each well. Mix well. Cover and incubate for 1 hour at room temperature.
4. Wash the Microtiter Plate using one of the specified methods indicated below:

Manual Washing: Remove incubation mixture by aspirating contents of the plate into a sink or proper waste container. Using a squirt bottle, fill each well completely with Wash Buffer (1X) then aspirate contents of the plate into a sink or proper waste container. Repeat this procedure four more times for a **total of FIVE washes**. After final wash, invert plate, and blot dry by hitting plate onto absorbent paper or paper towels until no moisture appears. *Note:* Hold the sides of the plate frame firmly when washing the plate to assure that all strips remain securely in frame.

Automated Washing: Aspirate all wells, then wash plates **FIVE times** using Wash Buffer (1X). Always adjust your washer to aspirate as much liquid as possible and set fill volume at 350 μ L/well/wash (range: 350-400 μ L). After final wash, invert plate, and blot dry by hitting plate onto absorbent paper or paper towels until no

moisture appears. *It is recommended that the washer be set for a soaking time of 10 seconds or shaking time of 5 seconds between washes.*

5. Add 100 μ l of Avidin Conjugate to each well. Cover and incubate for 1 hour at room temperature.
6. Prepare Substrate Solution no more than 15 minutes before end of second incubation (see Preparation of Reagents).
7. Repeat wash procedure as described in Step 4.
8. Add 100 μ L Substrate Solution to each well. Cover and incubate for 15 minutes at room temperature.
9. Add 100 μ L Stop Solution to each well. Mix well.
10. Read the Optical Density (O.D.) at 450 nm using a microtiter plate reader set within 30 minutes.

CALCULATION OF RESULTS

The standard curve is used to determine the amount of IL-4 in an unknown sample. The standard curve is generated by plotting the average O.D. (450 nm) obtained for each of the standard concentrations on the vertical (Y) axis versus the corresponding IL-4 concentration (pg/mL) on the horizontal (X) axis.

1. First, calculate the mean O.D value for each standard and sample. All O.D. values are subtracted by the value of the zero-standard (0 pg/mL) before result interpretation. Construct the standard curve using graph paper or statistical software.
2. To determine the amount of IL-4 in each sample, first locate the O.D. value on the Y-axis and extend a horizontal line to the standard curve. At the point of intersection, draw a vertical line to the X-axis and read the corresponding IL-4 concentration. If samples generate values higher than the highest standard, dilute the samples with the appropriate Calibrator Diluent and repeat the assay, the concentration read from the standard curve must be multiplied by the dilution factor.


TYPICAL DATA

Results of a typical standard run of a IL-4 ELISA are shown below. Any variation in standard diluent, operator, pipetting and washing technique, incubation time or temperature, and kit age can cause variation in result. The following examples are for the purpose of illustration only, and should not be used to calculate unknowns. Each user should obtain their own standard curve

EXAMPLE ONE


The following data was obtained for a standard curve using Calibrator Diluent I.

Standard (pg/mL)	O.D. (450 nm)	Mean	Zero Standard Subtracted (Std.)-(S1)
0	0.046, 0.044	0.045	0
31.25	0.128, 0.132	0.130	0.085
62.5	0.213, 0.221	0.217	0.172
125	0.386, 0.387	0.387	0.342
250	0.690, 0.714	0.702	0.657
500	1.195, 1.233	1.214	1.169
1000	1.889, 1.957	1.923	1.878

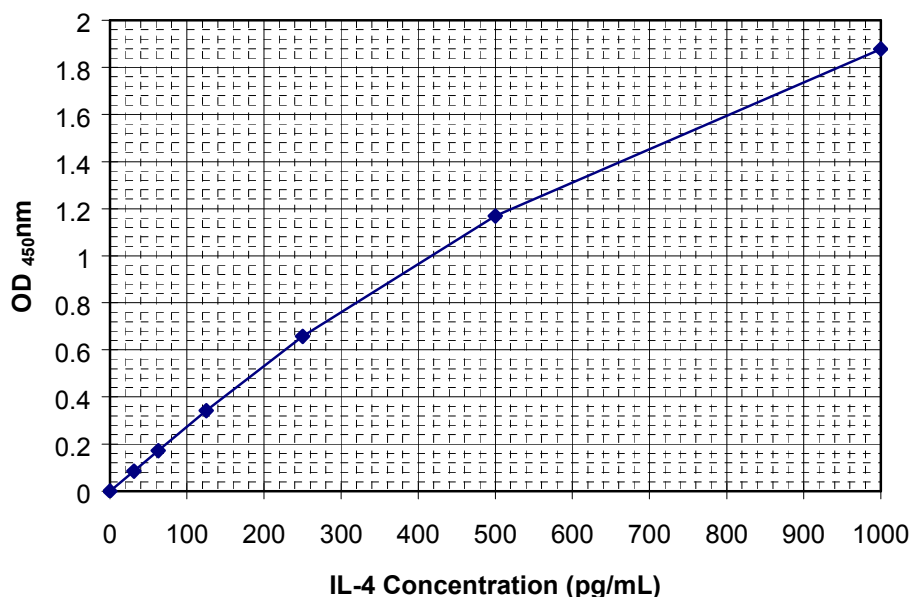**EXAMPLE TWO**

The following data was obtained for a standard curve using Calibrator Diluent II.

Standard (pg/mL)	O.D. (450 nm)	Mean	Zero Standard Subtracted (Std.)-(S1)
0	0.045, 0.037	0.041	0
31.25	0.153, 0.144	0.149	0.108
62.5	0.220, 0.235	0.228	0.187
125	0.371, 0.385	0.378	0.337
250	0.696, 0.708	0.702	0.661
500	1.208, 1.236	1.222	1.181
1000	1.996, 1.924	1.960	1.919

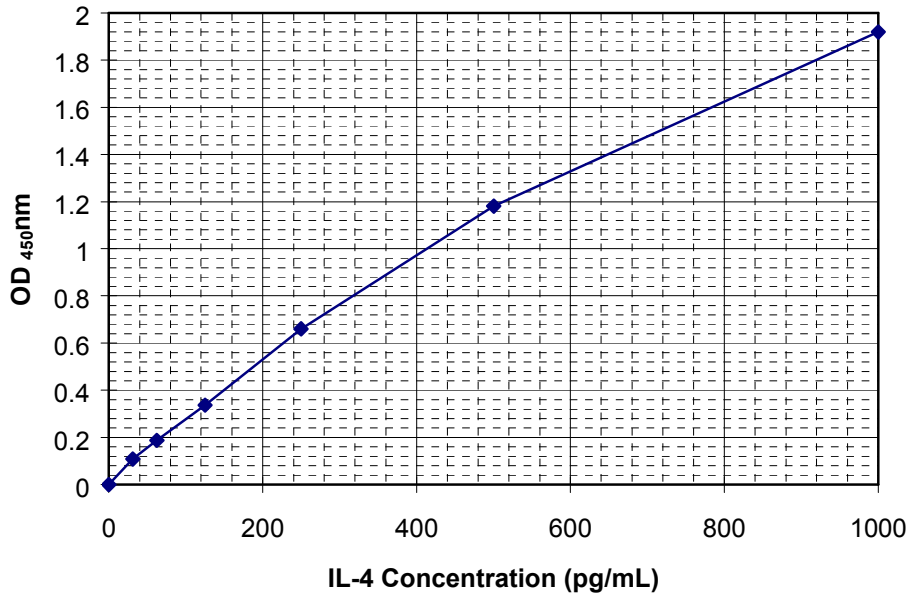

PERFORMANCE CHARACTERISTICS

1. INTRA-ASSAY PRECISION

To determine within-run precision, three different samples of known concentration were assayed by replicates of 20 in 1 assay.

Sample	Calibrator Diluent I assay			Calibrator Diluent II assay		
	1	2	3	1	2	3
n	20	20	20	20	20	20
Mean (pg/mL)	90	440	755	90	440	755
Standard Deviation (pg/mL)	6.6	29.9	47.6	5.9	22.4	39.3
Coefficient of Variation (%)	7.3	6.8	6.3	6.6	5.1	5.2

2. INTER-ASSAY PRECISION

To determine between-run precision, three different samples of known concentration were assayed by replicates on 20 different assays.

Sample	Calibrator Diluent I assay			Calibrator Diluent II assay		
	1	2	3	1	2	3
n	20	20	20	20	20	20
Mean (pg/mL)	111	432	786	111	432	786
Standard Deviation (pg/mL)	9.4	27.3	52.6	8.3	30.8	45.5
Coefficient of Variation (%)	8.4	6.3	6.7	7.6	7.1	5.8

3. **RECOVERY**

The recovery of IL-4 spiked to 3 different levels in sample throughout the range of the assay was evaluated.

Sample Type	Average Recovery %	Range %
Cell culture media	105	83 - 109
Serum	98	83 - 110
Plasma	90	80 - 108

4. **SENSITIVITY**

The minimum detectable dose of IL-4 was determined by adding two standard deviations to the mean optical density value of 20 zero standard replicates and calculating the corresponding concentration from the standard curve. The minimum detectable dose of human IL-4 using a standard curve generated with Calibrator Diluent I is 6.6 *pg/mL* and using Calibrator Diluent II is 4.3 *pg/mL*.

5. **SPECIFICITY**

This sandwich ELISA recognizes both natural and recombinant human IL-4. This kit exhibits no detectable cross-reactivity with human; SAA, EGF, IL-8, IL-16, MCAF, MCP-3, TNF- γ , M-CSF, GM-CSF, TGF- β_1 , RANTES, FGF, MIP-1 α , CRP, EPO, IFN- γ .

6. **CALIBRATION**

This immunoassay is calibrated against WHO Standard (First International Standard, 1994. Code No.: 88/656).

7. **EXPECTED NORMAL VALUES**

Biological samples from apparently healthy, normal individuals were collected and the average IL-4 concentration was measured. Serum/plasma samples (n=20) averaged less than the lowest IL-4 standard 31.25 *pg/mL*.

REFERENCES:

1. Howard, M. et al.(1982) J. Exp. Med. 155:914
2. Vitetta, E. S. et al.(1985) J. Exp. Med. 162:1726
3. Park, L. S. et al.(1987) J. Exp. Med. 166:476
4. Estes, M. L. et al.(1993) Am. J. Pathol. 143:337
5. Lacey, D. L. et al. (1993) J. Cell. Biochem. 53:122
6. Cabrillant, H. et al. (1987) Biochem. Biophys. Res. Commun. 149:995
7. Ohara, J. and W. E. Paul (1987)Nature 325: 537
8. Lowenthal, J. W. et al. (1988) J. Immunol. 140:456
9. Mosmann, T. R. and K. W. Moore (1991) Immunol. Today 12:A49
10. del Prete, G. et al. (1994) Lab Invest. 70:299
11. Sideras, P. et al. (1988) Proc. Natl. Acad. Sci. USA 85:218
12. Seder, R. A. et al. (1992) J. Immunol. 148:1652
13. Braddig, P. et al. (1992) J. Exp. Med. 176:1381
14. MacGlashan, D. et al. (1994) J. Immunol. 152:3006
15. Paul, W. E. et al. (1991) Blood 77:1859
16. Banchereau, J. and M.E. Rybak (1994) "Interleukin 4": in The Cytokine Handbook, 2nd ed. , A. Thomson, Ed. Academic Press, New York, p. 99
17. Carr. C. et al. (1991) Biochemistry 30: 1515
18. Zurawski, G. and J. E. de Vries (1994) Stem Cells 12:169
19. Walter, M. R. et al. (1992) J. Biol. Chem. 267:20371
20. D'Eustachio. P. et al. (1988) J. Immunol. 141:3067
21. Mosmann, T. R. and R. L. Coffman (1989) Annu. Rev. Immunol. 7:145
22. Tepper, R. I. et al. (1989) Cell 57:503
23. Urban, J. et al. (1991) Proc. Natl. Acad. Sci. USA 88:5513
24. Heinzl, F. et al. (1989) J. Exp. Med. 169:59
25. Sadick, M. D. et al. (1990) J. Exp. Med. 171:115

CITATIONS:

1. Sarchielli P et al. Proinflammatory cytokines, adhesion molecules, and lymphocyte integrin expression in the internal jugular blood of migraine patients without aura assessed ictally. Headache. 2006 Feb;46(2):200-7.
2. LIN-LIN WANG et al. Expression of CD39 mRNA is altered in the peripheral blood of patients with allergic asthma. Biomed Rep. Jan 2014; 2(1): 75–78.